

Sample Received: August 6, 2026

COA Issued: August 12, 2026

PRODUCT INFORMATION

Vendor:	Sample Name:	Sample Type:	Lot Number:	MW (g/mol):
Bacteriostatic Water Lab	Bacteriostatic Water 10mL	Clear liquid	0826bac10	91.1


ANALYTICAL METHODS

Identity: Confirmed via LC-MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Bacteriostatic Water	Benzyl Alcohol	LC-MS	✓ Conforms
Content	1.003 %	HPLC Quantitation	✓ Conforms
Overall Purity	99.83%	RP-HPLC (214 nm)	✓ Conforms
pH	6.25	pH Meter	✓ Conforms

HPLC Chromatogram (Retention Time: 5.940 min)

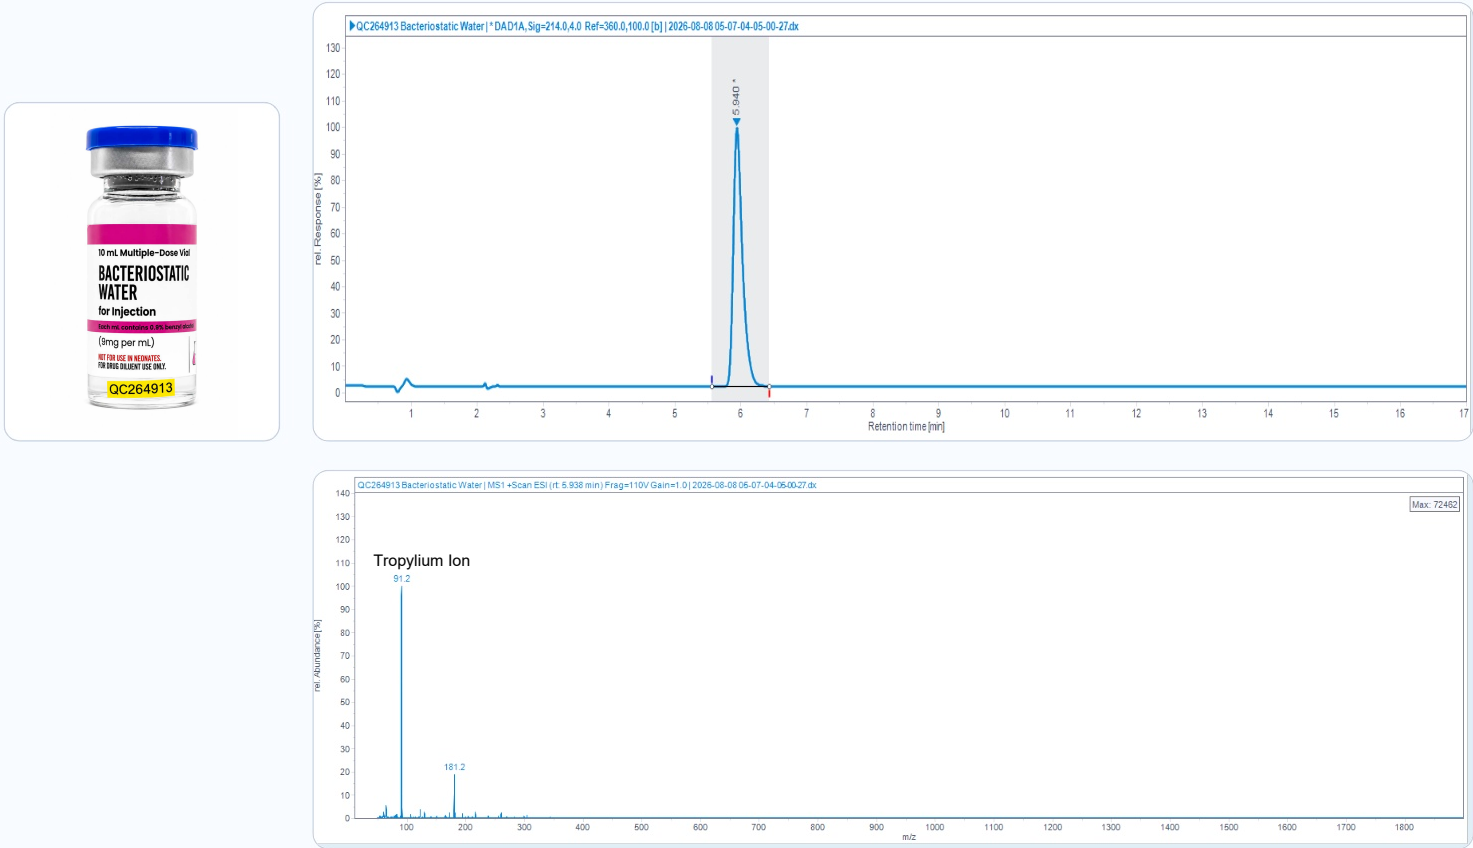

Certification: This COA confirms that the tested material meets or exceeds Bioviridian’s analytical quality specifications for peptide research use.
Visit: <https://bioviridians.com/coa-search.html>



Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.